

# HFRR Humidity Cabinet; Temperature Control Unit (TCU)

## Changes to the ISO 12156 Standard

We have developed the TCU to ensure all our customers can meet the revised ISO 12156 requirements even in extreme lab conditions.

We anticipate the revised standard to be published later this year with the main changes being the **tighter** limits for temperature and humidity ranges – see Figure 1 for full details.

To follow the progress of the ISO revision please see the ISO website: <https://www.iso.org/standard/72481.html>

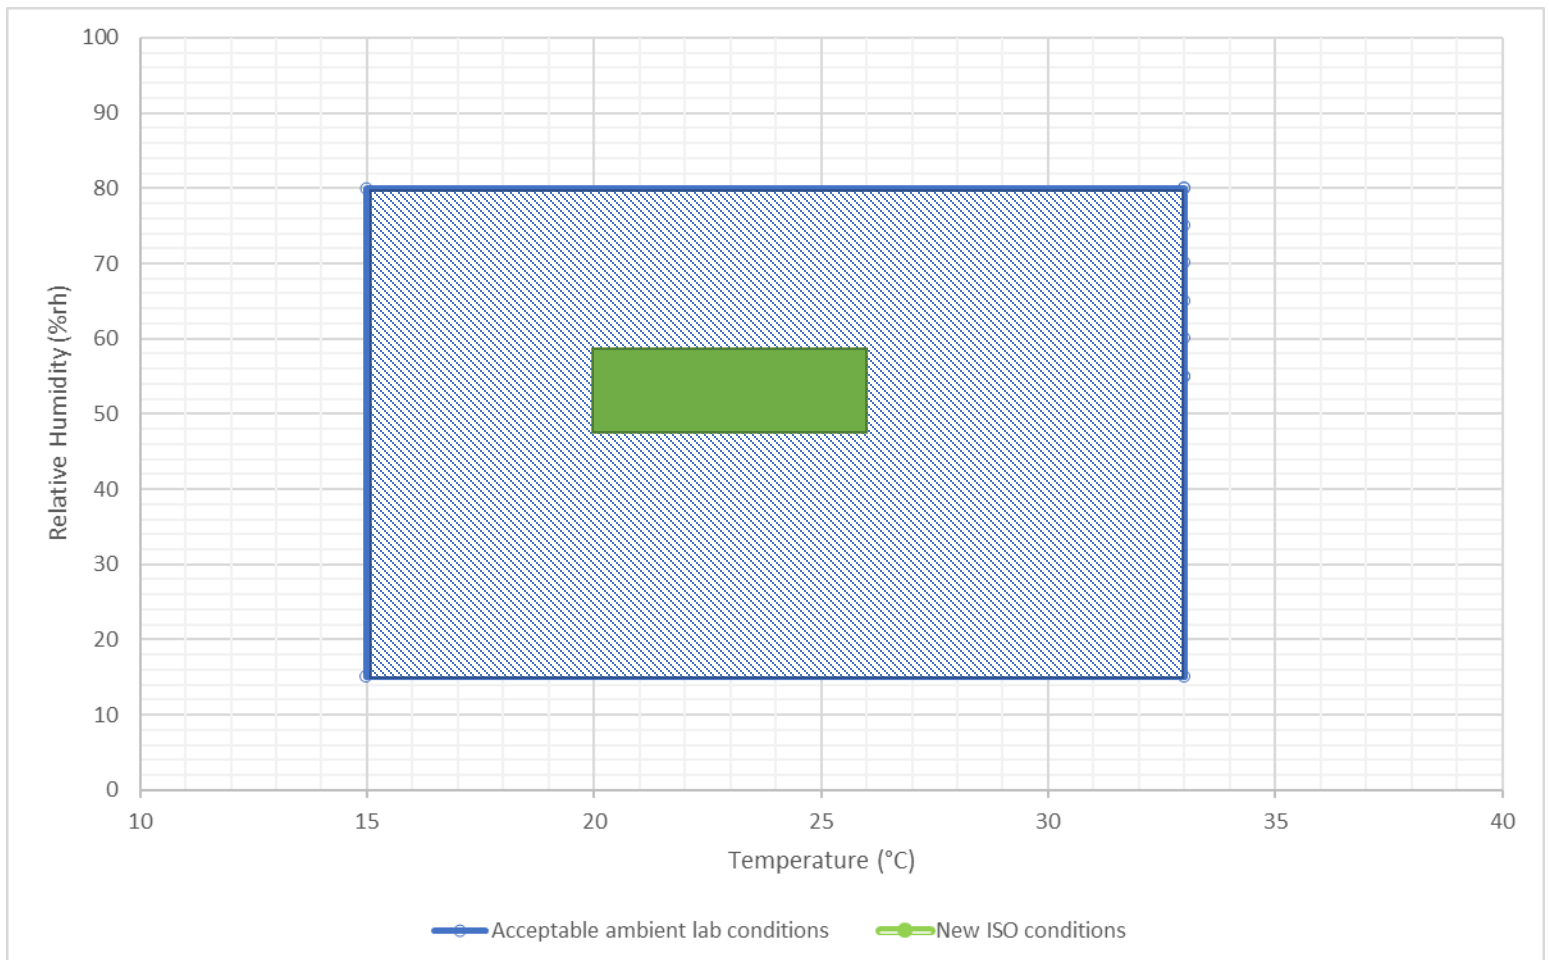


Figure 1: Revised ISO limits



## **Purchasing options**

Below is a comprehensive list of all the options we offer for the humidity cabinet and TCU. For further information and pricing please contact your local distributor.

Part Number	Title
PCS-003512	Complete Humidity Cabinet with TCU
PCS-003534	Retrofit Temperature Control Unit
PCS-002799 (HFRHCAB)	Humidity controlled cabinet for HFRR
PCS-003553	Temperature Control Unit